

**"Kurin Jet"**

CE Provider: Dept. for Behavior Health, Developmental and Intellectual Disabilities

KBN Provider-Training Number: 5-0051-0126-753




---

---

---

---

---



---

---

---

### What is Kurin?

- Market Leading Initial Specimen Discard Technology
- Reduces contaminated blood culture collections
- Passive, no required activation
- Easy to use/remain compliant
- Sidelines only first 0.15ml blood
- Does not change technique
- Zero Backorders or Shortages

---

---

---


---

---

---

---

---

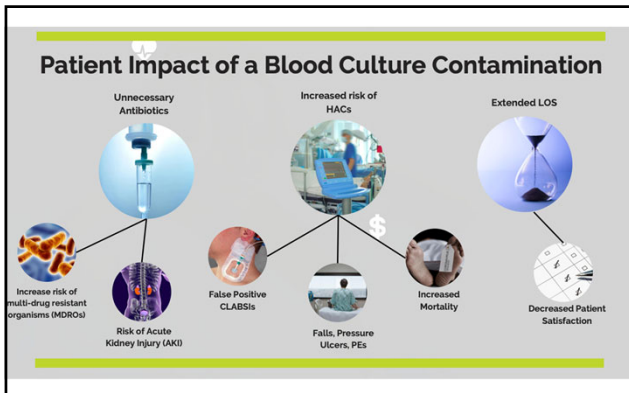


---

---

---

---

---

---


---

---



**"Kurin Jet"**

CE Provider: Dept. for Behavior Health, Developmental and Intellectual Disabilities

KBN Provider-Training Number: 5-0051-0126-753

 Addressing the New <1% Target

**Kurin® Your Only Passive Device to Meet CDC, CLSI, and INS Guidelines for Preventing Blood Culture Contaminations**

**kurin®**  
**JET**

**CLINICAL AND LABORATORY STANDARDS INSTITUTE**

---

---

---

---


---

---

---

---

**Market Leading Kurin® Clinical Outcomes Team**  
Service and Support for Proven Results



**Needs Analysis**   **Planning Meeting**   **Implementation**   **Feedback Loop**

**kurin®**

---

---

---

---

---

---

---

---

**Watch Kurin in Action**



**kurin®**

---

---

---

---

---

---

---

---

"Kurin Jet"

CE Provider: Dept. for Behavior Health, Developmental and Intellectual Disabilities

KBN Provider-Training Number: 5-0051-0126-753

Configured for ease of use, **Kurin JET™** offers options for all blood culture collection methods.

Venipuncture



Syringe Draws



Freshly-Placed PIVs



**Kurin® Jet™ Ordering Information (200/cs)**  
 Venipuncture Collection Sets with Push-Button Needles  
 21 gauge and 23 gauge, with adapter for BD Bactec®, bioMérieux BacT/Alert®, or ThermoFisher REDOX™  
 Peripheral IV Collection Sets  
 Fits BD Bactec®, bioMérieux BacT/Alert®, or ThermoFisher REDOX™




---

---

---

---


---

---

---


---

FDA 510(k) Clearances



- K220677
  - Indicated for blood culture collection & to reduce blood culture contamination rates\*
- Additional 510k
  - K162233 – Initial approval for butterfly needle technology
  - K181895 – Approval for IV Connection
  - K191832 – Approval for Advance safety needle technology

\*The Kurin Blood Collection System is for use as a blood collection system and its Bure Lock allows the aspiration of blood from the patient to be inhibited prior to the collection of the test sample to reduce the frequency of blood culture contamination when contaminants are present in the initial blood sample compared to blood culture drawn using standard practice without the Kurin Lock.




---

---

---

---


---

---


---

---


FDA 510(k) Clearances



- Following FDA guidance document, Jet is covered under Kurin existing 510(k)'s
- All Kurin Jet product codes registered with FDA GUDID database



<https://www.access.gpo.gov/cg-bin/xis/govdocs/search/query.pl?qs=documents/decidingwhen-submit-510k-change-existing-device>  
<https://www.fda.gov/registry-information/search-fda-guidance-documents/decidingwhen-submit-510k-change-existing-device>




---

---

---

---

---

---


---

---

***“Kurin Jet”***

CE Provider: Dept. for Behavior Health, Developmental and Intellectual Disabilities

KBN Provider-Training Number: 5-0051-0126-753

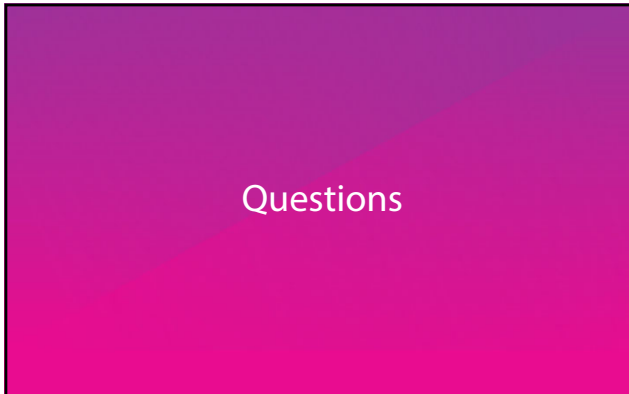

---

---

---

---

---

---

---

---